

Please answer all questions directly on exam paper. Each question is worth 20 points.

Name: Answers Student number: 000006

VERSION B

1. a) What are the main advantage and the main disadvantage of using axial viewing detection in ICP-OES?
- b) What is the role of the nebulization chamber in ICP-OES instruments?
- c) Why not measure the absorbance of elements rather than their emission in the plasma torch?

- a) advantage: more sensitivity, as more light is viewed.
disadvantage: less selectivity, as no height adjustment is possible.
- b) To select droplets by size from the nebulizer. Only the smallest droplets will reach the plasma.
- c) In absorbance measurements, a mono λ light goes through a sample of known pathlength and transmittance is measured, along the axis of the incident light. In ICP OES, the torch is so intense that along the same axis it is impossible to detect a T change whether the sample is in or not. The sample is the light source in this experiment as emission is recorded.

2. a) Four standard solutions are measured by UV spectrophotometry at 254 nm, of concentrations 1, 2, 4 and 8 mg/mL with corresponding absorbance values of 0.02, 0.04, 0.08, and 0.16. What is the path length of the measuring cuvette if the correlation coefficient (slope) is $0.04 \text{ mL}^{-1} \text{ cm}^{-1}$?
- b) Which cuvette material would be best to use, polyvinyl chloride (PVC), quartz, or ordinary glass? Justify.

a) The slope obtained by the measurements is $0.02 \text{ mL}^{-1} \text{ cm}^{-1}$




If the cell length is 1 cm, the coefficient obtained was 0.04
 \Rightarrow the cell has $\frac{1}{2}$ the length, $\Rightarrow 0.5 \text{ cm}$

b) Quartz is the most transparent in the 254 nm range - Glass has metal ions that cause absorbance in that range and PVC is an organic polymer, likely to cause a high background at that wavelength.


3. a) By drawing/writing on the atomic energy diagram given below (left section), show what happens during an X-ray photoelectron emission event.

b) On the right section of the diagram, draw vertical arrows to indicate the binding energy of the electrons in that particular atom.

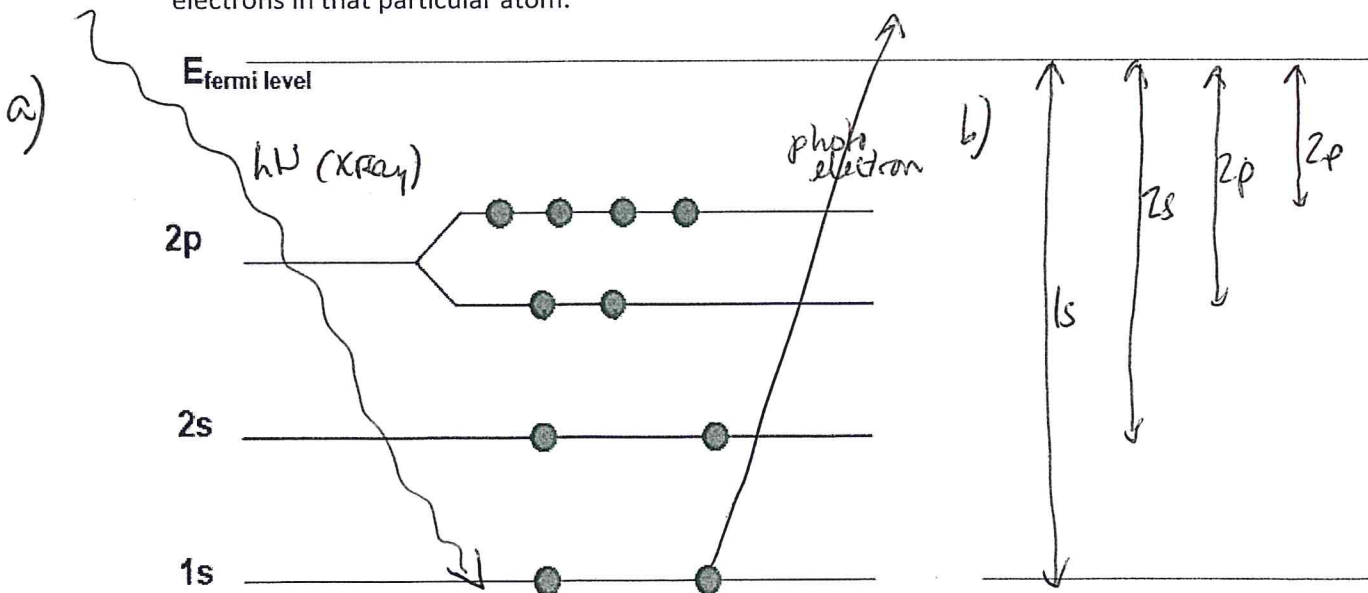

4. A 8-g sample of lead carbonate (PbCO_3) is dropped into a 100-L beaker of water. The pH is adjusted to 5 with formic acid (HCOOH). The K_{sp} of lead carbonate is 7.4×10^{-14} .

- Calculate the Pb^{2+} concentration at equilibrium.
- Would it be possible to lower the pH enough to dissolve the whole sample?

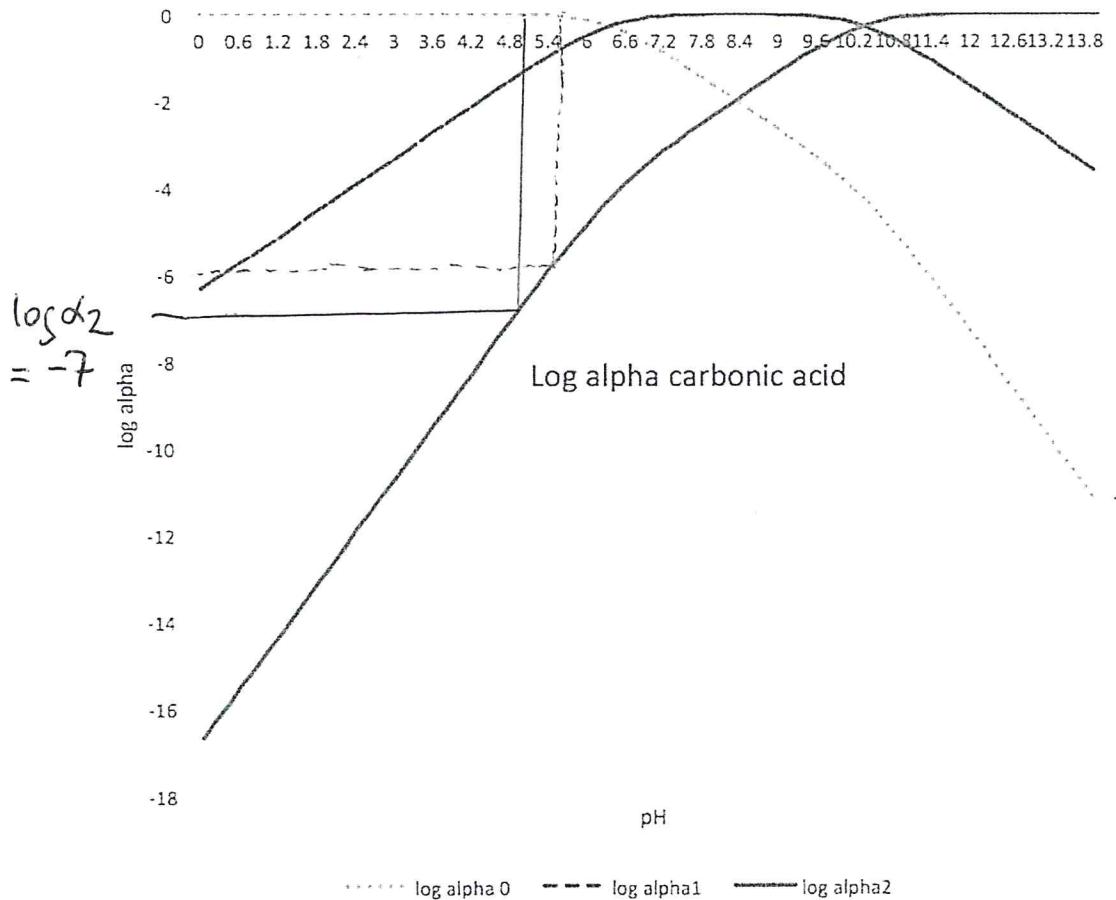


a) $\alpha_2 = 10^{-7}$ $[\text{Pb}^{2+}] = \sqrt{\frac{K_{sp}}{\alpha_2}} = \sqrt{\frac{7.4 \times 10^{-14}}{10^{-7}}} = 8.6 \times 10^{-4} \text{ M}$

b) Whole sample: $\frac{8 \text{ g}}{267 \text{ g/mol}} = 3 \times 10^{-2} \text{ mole}$, $[\text{Pb}^{2+}] = \frac{3 \times 10^{-2}}{100 \text{ L}} = 3 \times 10^{-4} \text{ M}$

By dissolving the whole sample, we get a lower conc. than in a) meaning that at pH 5 it is already all dissolved.

at $\alpha_2 = \frac{K_{sp}}{[\text{Pb}^{2+}]^2} = \frac{7.4 \times 10^{-14}}{(3 \times 10^{-4})^2} = 8.2 \times 10^{-7}$, $\log \alpha_2 = -6.08$ $\text{pH} \approx 5.6$ is needed to

5. a) Given that the radius of Cd^{2+} trajectory in a constant field SIMS magnetic analyzer is 30 cm, calculate the distance between the detection points of Cd^{2+} , Al^{3+} and K^+ after a 180° trajectory. Use the diagram below as example for guidance.

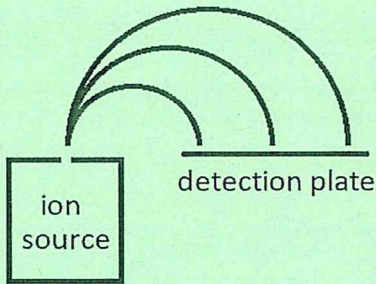

b) Primary ions (Cs^+ , O_2^+) strike the sample for ejection of secondary ions from the analyte: Pb^{2+} , Al^{3+} , Na^+ .

b) Why are Cd^{2+} , Al^{3+} and K^+ called secondary ions?

$$m/z = \text{constant} \times R^2$$

a/ for Cd^{2+} : $\frac{112}{2} = c \times (35)^2 \Rightarrow c = 0.046$

Al^{3+} : $\frac{27}{3} = 0.046 \times R^2 \Rightarrow R = 14 \text{ cm}$

K^+ : $\frac{39}{1} = 0.046 \times R^2 \Rightarrow R = 29 \text{ cm}$

